


Oscilloscope-XSC1

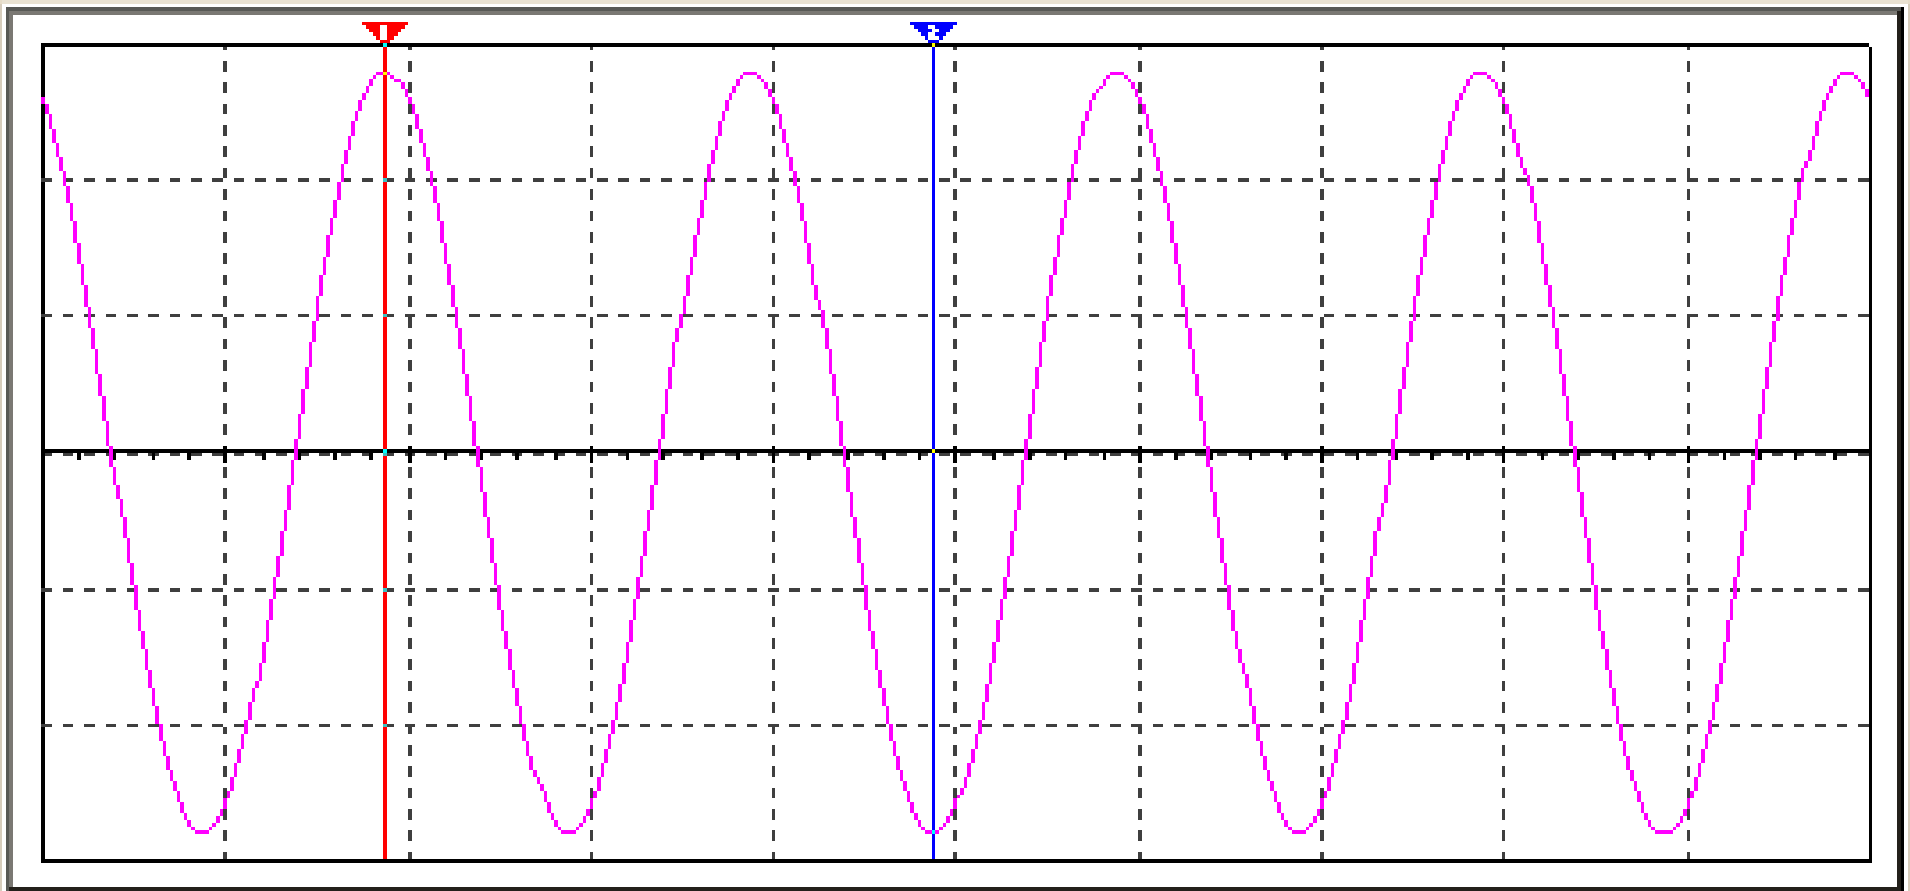

T1	← →	Time	Channel_A	Channel_B	Reverse
T2	← →	411.253 ms	27.989 V		
T2-T1		412.753 ms	-27.989 V		Save
		1.500 ms	-55.978 V		Ext. Trigger

Timebase	Channel A	Channel B	Trigger
Scale 500 us/Div	Scale 10 V/Div	Scale 5 V/Div	Edge F Z A B Ext
X position 0	Y position 0	Y position 0	Level 0 V
Y/T Add B/A A/B	AC 0 DC	AC 0 DC -	Type Sing. Nor. Auto None