


Startfreq: 0.400000 MHz; Stopfreq: 0.499900 MHz; Stepwidth: 0.100 kHz

Samples: 1000; Interrupt: 0 uS

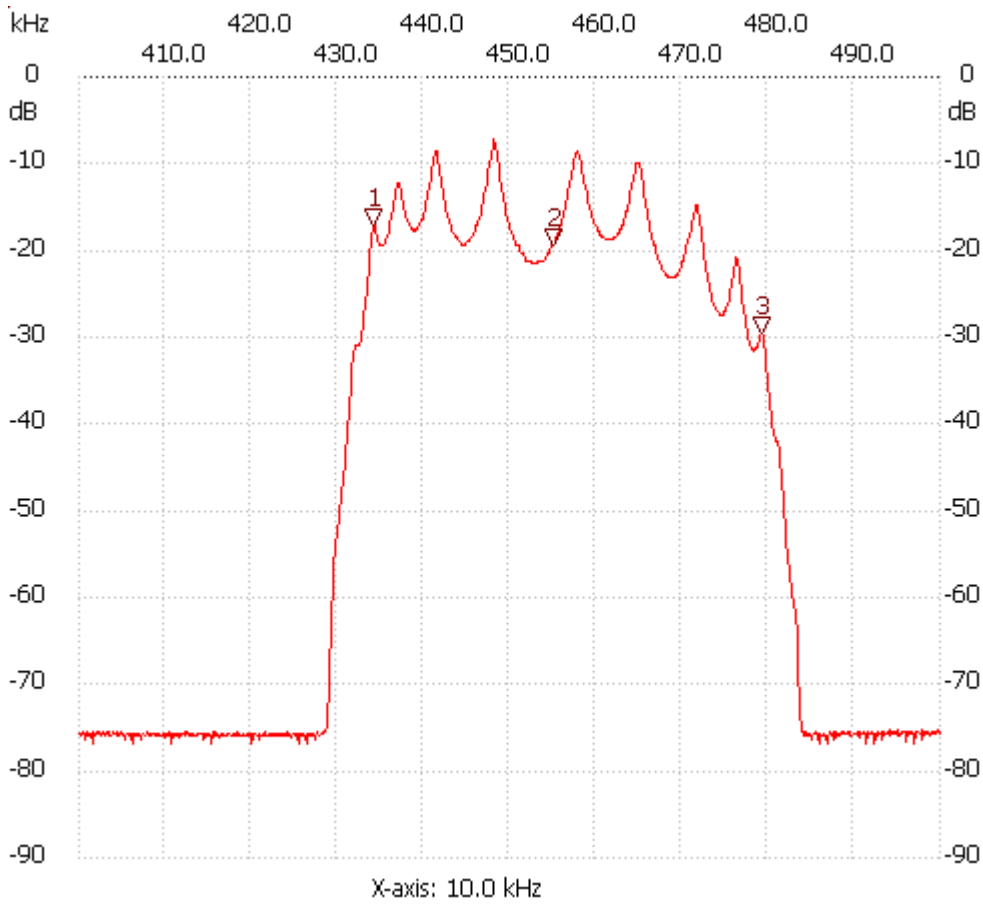

;CFS-455 455KHz-es szűrő

Cursor 1:

0.434200 MHz

Channel 1: -17.06dB

Cursor 2:

0.455100 MHz

Channel 1: -19.28dB

Cursor 3:

0.479200 MHz

Channel 1: -29.48dB

Channel 1

max :-7.23dB 0.448200MHz

min :-76.96dB 0.401600MHz